

DG Filters 700 Series Refilling Instructions



DG Filter 700 S Refilling Instructions

Chemteq, Inc.
600 West 24th Street, Suite B
Norfolk, Virginia 23517
USA

<http://www.chemteq.net>

Tel: 757-622-2223 / Toll free: 855-CHEMTEQ

NOTICES

These instructions are prepared exclusively for the owner of Chemteq DG Filters 700 Series (DG Filters 700 S). The content of these instructions is proprietary information and are to be used only to understand, refill and maintain the DG Filters 700 S. By receiving this document, the recipient agrees that neither this document nor the information disclosed within nor any part hereof shall be reproduced or transferred, physically, electronically or in any other form, or used or disclosed to others for manufacturing or for any other purpose except as specifically authorized in writing by Chemteq, Inc.

© 2009 Chemteq, Inc. All Rights Reserved. No part of this document may be reproduced, transmitted, transcribed, stored in a retrieval system, or translated into any language in any form by any means without the prior written permission of Chemteq, Inc.

The information in this document is subject to change without notice. The images and drawings used in these instructions are for explanatory purposes only and may not be identical with the actual device in their appearance, size, color or positions.

Chemteq is registered trademark of Chemteq, Inc.

DG Filters 700 Series are manufactured by Chemteq.

Made in the United States of America



CAUTIONS

READ AND UNDERSTAND ALL INSTRUCTIONS BEFORE USE

1. These Instructions must be read and understood by user before operating this product or using its accessories, in order to ensure proper and safe use of this product.
2. Read and understand all applicable federal, state, and local environmental health and safety laws and regulations, including OSHA. Ensure complete compliance with all applicable laws and regulations before and during use of this product.
3. Do not substitute, modify, or omit parts or components. Use exact manufactured replacement parts in configurations specified by the original manufacturer.
4. Contact Chemteq's Service Department for any questions regarding these instructions or to arrange for a Returned Material Authorization (RMA).

Table of Contents

TABLE 1: COMPONENTS OF THE DG FILTERS 700 S REFILL KIT 1

TABLE 2: DG FILTERS 700 SERIES SORPTION MEDIA 1

1. INSTRUCTIONS 2

1.1. REMOVE FIXATION SCREW (FIGURE 2) 2

1.2. REMOVE REFILL CAP (FIGURE 3) 3

1.3. REMOVE FELT (FIGURES 4 & 5) 3

1.4. REMOVE STAINLESS STEEL SCREEN (FIGURE 6 & 7) 3

1.5. EMPTY EXHAUSTED SORPTION MEDIA (FIGURE 8) 4

1.6. CHARGE FILTER WITH FRESH SORPTION MEDIA (FIGURE 9) 4

1.7. REPLACE STAINLESS STEEL SCREEN AND FELT (FIGURES 10 & 11) 4

1.8. REPLACE REFILLING CAP (FIGURE 12) 5

1.9. REPLACE FIXATION SCREW (FIGURE 13) 5


Table 1: Components of the DG Filters 700 S Refill Kit

Item No.	Description	No. of Items	Part Number
1	Sorption Media	1	See table 2 for specific refill kit
2	Screen & felt set	1	Optional

Table 2: DG Filters 700 Series Sorption Media

Item No.	Refill Kit	No. of Items	Part Number
1	Acids	1	721-1000
2	Allyl bromide	1	764-1000
3	Ammonia	1	724-1000
4	Ammonia & hydrogen sulfide	1	727-1000
5	Aromatic diisocyanates	1	730-1000
6	Basic Vapors	1	733-1000
7	Chlorine Dioxide	1	742-1000
8	Formaldehyde	1	735-1000
9	Glutaraldehyde	1	736-1000
10	Halogens	1	738-1000
11	Hydrazine	1	745-1000
12	Hydrogen sulfide	1	740-1000
13	Mercaptans	1	754-1000
14	Mercury & Mercury II Compounds	1	455-1000
15	Nitrogen dioxide	1	756-1000
16	Organic Vapors	1	761-1000

Figure 1: Schematic Diagram of the DG Filter 700 Series

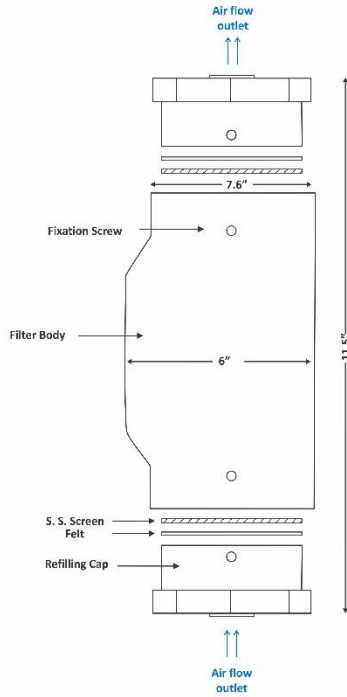

1. Instructions

1.1. Remove Fixation screw (Figure 2)



Figure 2

DG Filter 700 S Refilling Instructions

1.2. Remove refill Cap (Figure 3)



Figure 3

1.3. Remove felt (Figures 4 & 5)



Figure 4

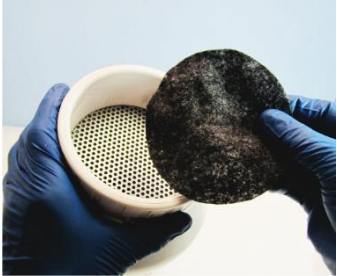


Figure 5

1.4. Remove stainless steel screen (Figure 6 & 7)

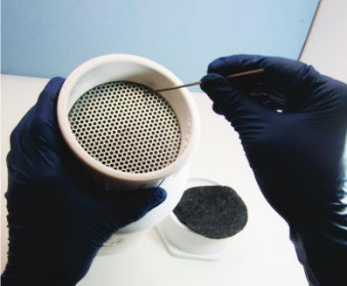


Figure 6

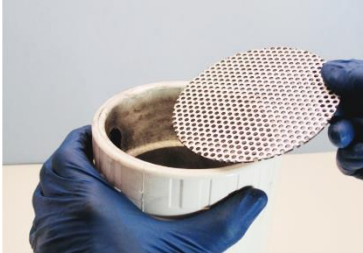


Figure 7

DG Filter 700 S Refilling Instructions

1.5. Empty exhausted sorption media (Figure 8)



Figure 8

1.6. Charge filter with fresh sorption media (Figure 9)

Occasionally shake filter during adding sorption media for uniform filling



Figure 9

1.7. Replace stainless steel screen and felt (Figures 10 & 11)

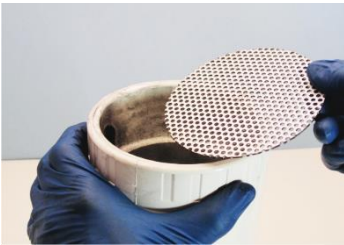


Figure 10

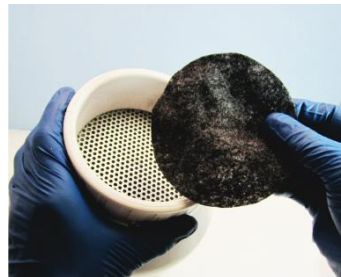


Figure 11

DG Filter 700 S Refilling Instructions

1.8. Replace refilling cap (Figure 12)

Ensure alignment of marking (a) on refilling cap with marking (b) on filter body (b).

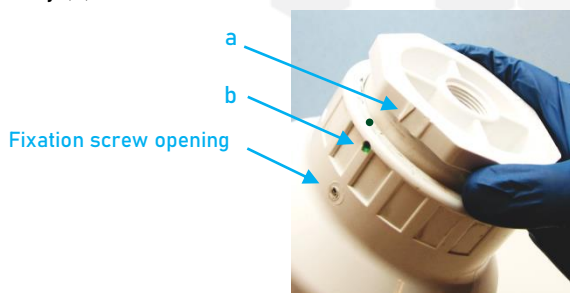


Figure 12

1.9. Replace fixation screw (Figure 13)



Figure 13

PLEASE CALL US AT 757-622-2223 OR EMAIL US AT info@chemteq.net
FOR ANY QUESTIONS REGARDING THESE INSTRUCTIONS



600 West 24th Street, Suite B, Norfolk, VA23517

Tel: 757-622-2223, Toll-free 855-243-6837 (855-CHEMTEQ)

Email: sales@chemteq.net

<http://www.chemteq.net>